


Principles of Safety and Performance for Medical Hyperbaric Chambers: Guidelines for Regulatory Submission

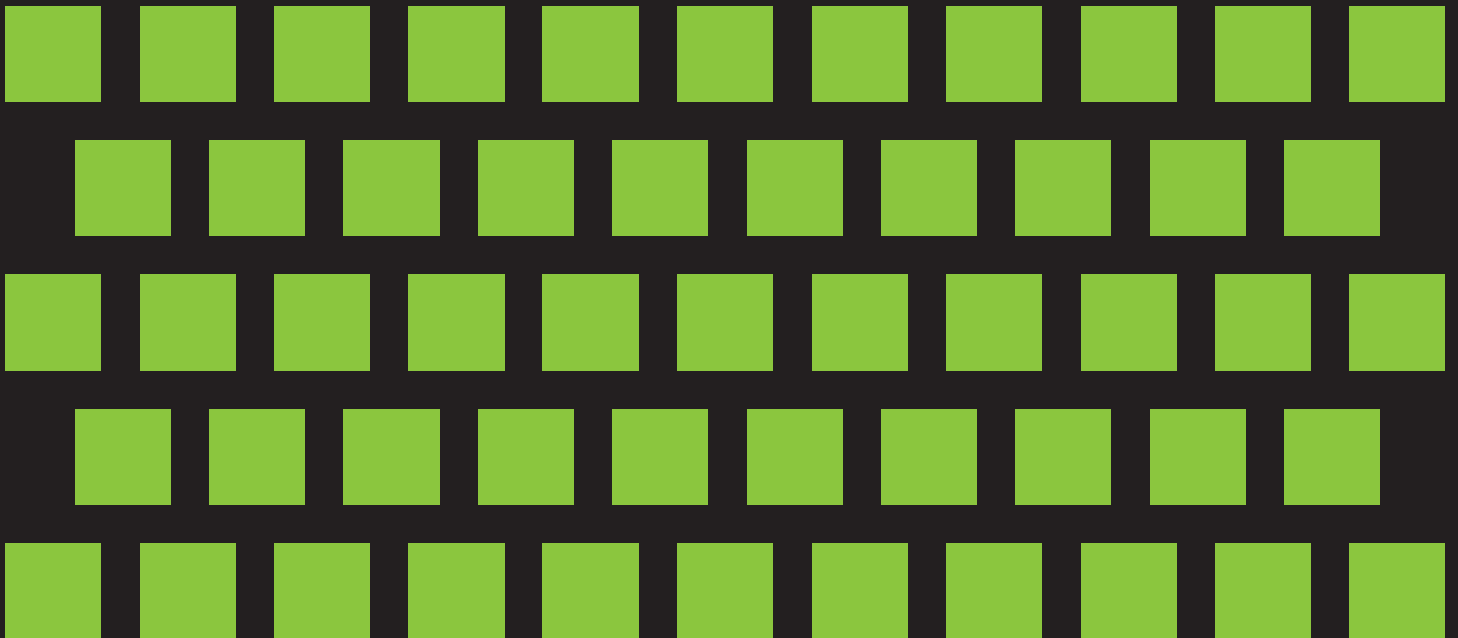

STP-PT-047

**PRINCIPLES OF SAFETY
AND PERFORMANCE FOR
MEDICAL HYPERBARIC
CHAMBERS:
GUIDELINES FOR
REGULATORY SUBMISSION**

Prepared by:

ASME PVHO Subcommittee
on Medical Hyperbaric Systems



Date of Issuance: June 30, 2011

This report was prepared as an account of work sponsored by ASME Pressure Technology Codes & Standards and the ASME Standards Technology, LLC (ASME ST-LLC).

Neither ASME, ASME ST-LLC, nor others involved in the preparation or review of this report, nor any of their respective employees, members or persons acting on their behalf, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness or usefulness of any information, apparatus, product or process disclosed, or represents that its use would not infringe upon privately owned rights.

Reference herein to any specific commercial product, process or service by trade name, trademark, manufacturer or otherwise does not necessarily constitute or imply its endorsement, recommendation or favoring by ASME ST-LLC or others involved in the preparation or review of this report, or any agency thereof. The views and opinions of the authors, contributors and reviewers of the report expressed herein do not necessarily reflect those of ASME ST-LLC or others involved in the preparation or review of this report, or any agency thereof.

ASME ST-LLC does not take any position with respect to the validity of any patent rights asserted in connection with any items mentioned in this document, and does not undertake to insure anyone utilizing a publication against liability for infringement of any applicable Letters Patent, nor assumes any such liability. Users of a publication are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, is entirely their own responsibility.

Participation by federal agency representative(s) or person(s) affiliated with industry is not to be interpreted as government or industry endorsement of this publication.

ASME is the registered trademark of the American Society of Mechanical Engineers.

No part of this document may be reproduced in any form,
in an electronic retrieval system or otherwise,
without the prior written permission of the publisher.

ASME Standards Technology, LLC
Three Park Avenue, New York, NY 10016-5990

ISBN No. 978-0-7918-3368-1

Copyright © 2011 by
ASME Standards Technology, LLC
All Rights Reserved

TABLE OF CONTENTS

Foreword v

Abstract vi

1 Scope..... 1

2 Device Description..... 2

3 General Safety Information..... 4

4 Essential Principles and Evidence of Conformity..... 5

 4.1 Materials..... 5

 4.1.1 Pressure Bearing Components..... 5

 4.1.2 Material Compatibility 5

 4.1.3 Toxicity 5

 4.1.4 Biocompatibility..... 5

 4.1.5 Sterility..... 5

 4.2 Specifications 5

5 Summary of Design Verification and Validation 7

 5.1 Materials..... 7

 5.1.1 Pressure Bearing Materials..... 7

 5.1.2 Biocompatibility..... 7

 5.1.3 Toxicity 7

 5.1.4 Material Compatibility 7

 5.2 Electro-Mechanical Safety 7

 5.2.1 Performance Testing of Hyperbaric Oxygen Chambers..... 7

 5.2.2 Pressure Vessel..... 7

 5.2.3 Pressurization / Depressurization System (Controls) 8

 5.2.4 Performance Criteria 8

 5.2.5 Controls Protection..... 8

 5.2.6 Connector Protective Incompatibility..... 8

 5.2.7 Medical Gas Connections..... 8

 5.2.8 Mechanical Safety 8

 5.2.9 Mechanical Vibration and Shock Resistance 9

 5.2.10 Fluid Spill Resistance..... 9

 5.2.11 High and Low Temperature and Humidity 9

 5.2.12 Surface Temperature 9

 5.2.13 Strangulation 9

 5.3 Electrical..... 9

 5.4 Software 10

 5.5 Visual and Audible Indicators and Alarms 10

 5.5.1 Power Indicators..... 10

 5.5.2 Visual and Audible Alarms 10

6 Clinical Evidence..... 11

7 Labeling 12

8 Risk Analysis 13

9 Manufacturer Information..... 14

Acknowledgments.....15
Abbreviations and Acronyms16

LIST OF TABLES

Table 1 - Example Hazards and Mitigation Table4

FOREWORD

In the United States, Hyperbaric Oxygen Therapy (HBOT) is considered to be a medical treatment and requires a physician's prescription. Furthermore, Hyperbaric Chambers intended to be used to administer HBOT treatments require Federal Drug and Food Administration's (FDA) approval. Similar regulatory submissions such as the Global Harmonization Task Force (GHTF) document "Summary Technical Documentation for Demonstrating Conformity to the Essential Principles of Safety and Performance of Medical Devices (STED)" are required in other countries.

This publication provides guidance for completing such regulatory submissions as well as principles of safety and performance of Pressure Vessels for Human Occupancy intended for use as medical devices. The FDA's regulatory submission package encourages compliance to the ASME PVHO-I Standard, and therefore compliance with the PVHO-I Standard requirements pertaining to the manufacture of Hyperbaric Chambers are recommended in this Guide.

The work contained in this publication was started in 2007 by the PVHO Subcommittee on Medical Hyperbaric Systems. The technical review was conducted by the ASME Pressure Vessel for Human Occupancy (PVHO) Committee over a period of three years. The PVHO Committee which conducted the technical review consists of twenty three members and two delegates representing several industry sectors which include manufacturers, users, insurance companies, regulatory and governmental agencies, as well as five countries: the USA, Canada, England, Germany and Australia.

Established in 1880, the American Society of Mechanical Engineers (ASME) is a professional not-for-profit organization with more than 127,000 members promoting the art, science and practice of mechanical and multidisciplinary engineering and allied sciences. ASME develops codes and standards that enhance public safety, and provides lifelong learning and technical exchange opportunities benefiting the engineering and technology community. Visit www.asme.org for more information.

The ASME Standards Technology, LLC (ASME ST-LLC) is a not-for-profit Limited Liability Company, with ASME as the sole member, formed in 2004 to carry out work related to newly commercialized technology. The ASME ST-LLC mission includes meeting the needs of industry and government by providing new standards-related products and services, which advance the application of emerging and newly commercialized science and technology and providing the research and technology development needed to establish and maintain the technical relevance of codes and standards. Visit www.stllc.asme.org for more information.

ABSTRACT

This document is intended to provide guidance with development, review and approval of regulatory submissions involving hyperbaric chambers. While there are specific standards and regulatory requirements for the design, production and regulatory approval of medical devices and pressure equipment, there has not been regulatory guidance for the evaluation of pressure vessels intended for use as medical devices. This document provides assistance for completing regulatory submissions such as the Global Harmonization Task Force (GHTF) document “Summary Technical Documentation for Demonstrating Conformity to the Essential Principles of Safety and Performance of Medical Devices (STED)” and the United States Food and Drug Administration’s (FDA) Premarket Notification process (510k).

1 SCOPE

This document applies to hyperbaric chambers intended for use as medical devices for the clinical treatment of various diseases and conditions. This document may also find application in related areas such as for hyperbaric chambers intended for medical research.